


Galvanic Isolator 3945 Conductivity, Temperature and Depth

An Interface between Recording Doppler Current Profiler RDCP 600 and Aanderaa equipment with PDC-4 input.

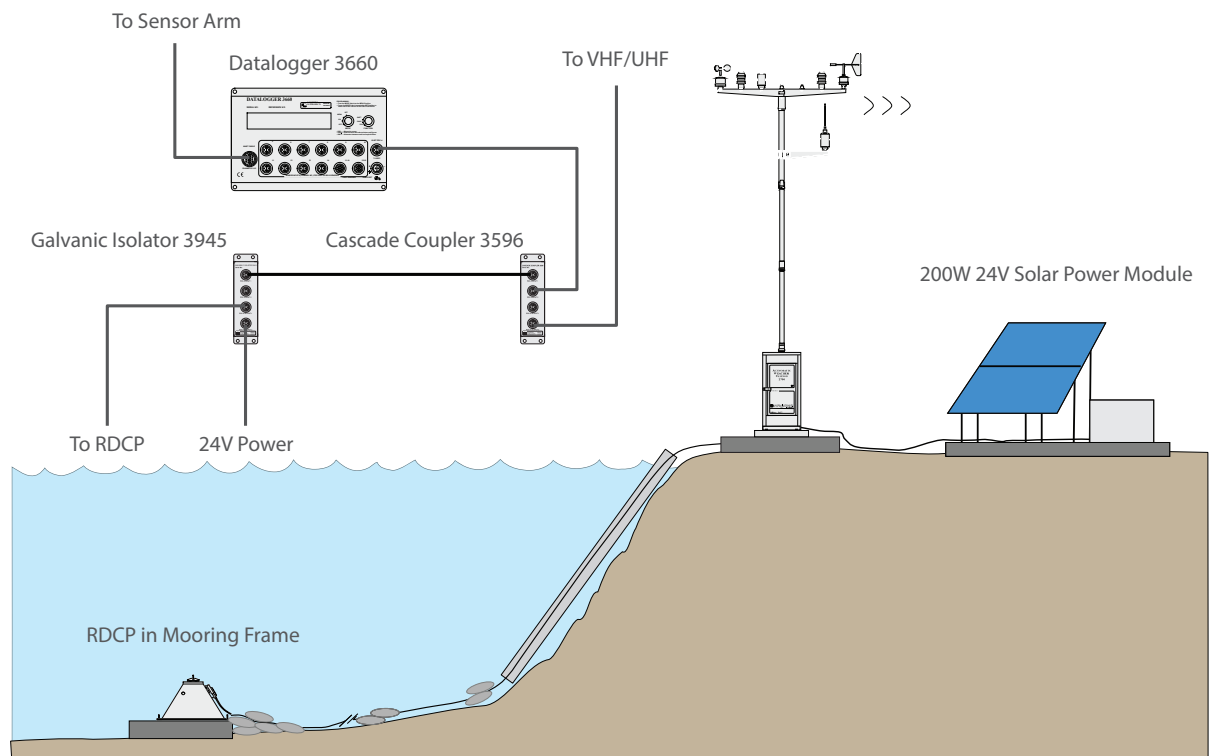


The Galvanic Isolator 3945 is to be used as an interface between a RDCP 600, configured to output data in PDC-4 format, and an Aanderaa device with PDC-4 input.

The input side and the output side are galvanically isolated from each other by use of optocouplers and an internal

DC/DC converter.

The DC/DC converter will convert the 24-48V DC input power to 12V DC output power that can be used to supply Aanderaa equipment connected to the output side with power.

SPECIFICATIONS

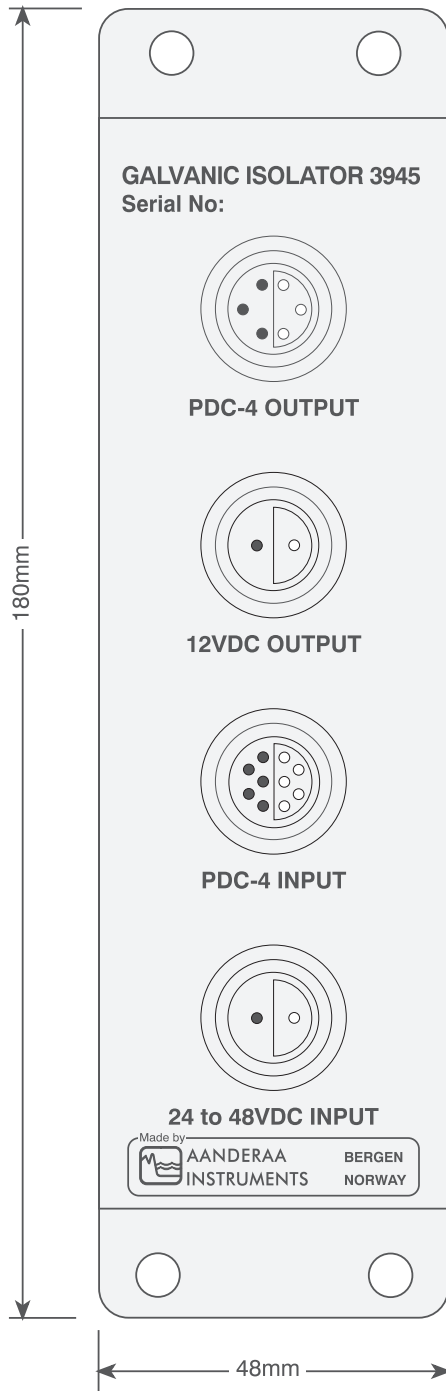





Input/Output Signals: Aanderaa PDC-4
 Operating Voltage: 18-50V
 Current Consumption: 18mA @ 24V
 Maximum Current Drain from 12V DC Out and PDC-4 Output: 400mA *
 Operating Temperature: -40 to +50°C
 Material Housing: Aluminum 6061T6 anodized 20µ
 Net Weight: 350 grams
 Packing: Cardboard Box: 385 x 290 x 235mm
 Gross Weight: 1.1 kilograms

* A built in DC/DC converter will supply equipment connected to the "PDC-4 Output" or the "12V DC Output" connector with limited power (12 VDC max. 400mA).

The "12V DC Output" connector can also be used as an power input if extra power is needed for equipment connected to the PDC-4 Output. Input voltage should be in the range 12 - 16VDC.

PIN CONFIGURATION

Receptacle, exterior view; bushing = ○, pin = ●

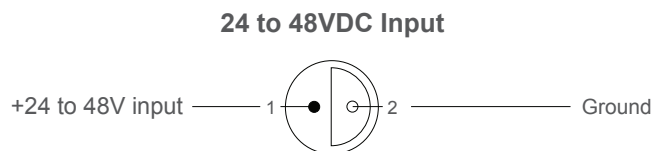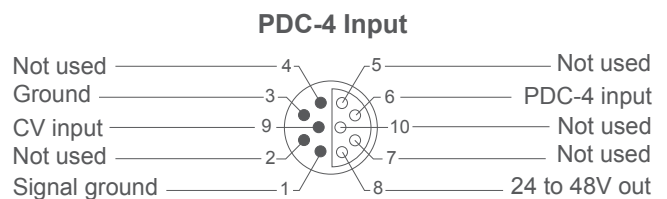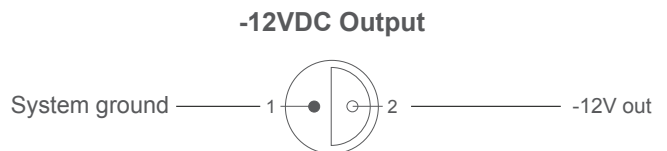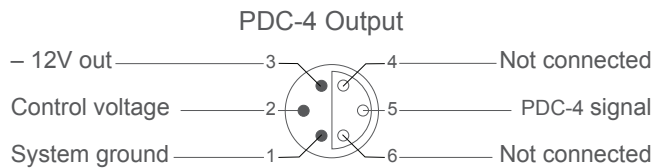

Visit our Web site for the latest version of this document and more information
www.aadi.no

Aanderaa is a trademark of Xylem Inc. or one of its subsidiaries.
 © 2012 Xylem, Inc. D369 January 2013

Aanderaa Data Instruments AS
 Sanddalsringen 5b, P.O. Box 103
 Midtun, 5828 Bergen, Norway
 Tel +47 55 60 48 00
 Fax +47 55 60 48 01