



The Data Storage Unit (DSU) is a portable, reusable, solid state module for storing data in the 10-bit PDC-4 code.

Data Storage Unit (DSU) is a standard data storage device for all Aanderaa Automatic Weather Stations, data collecting instruments and databuys with PDC-4 output.

The unit has a six-pin watertight receptacle for input/output of data. A five-digit LCD module shows the total number of data stored. After the unit is removed from an installation an internal battery provides power to the clock and LCD.

The DSU incorporates a pre-settable, real-time clock for recording time information. A time record consists of six ten-bit words. The first is a fixed binary reading equal to 7, followed by 5 words indicating year, month, day, hour and minute.

The DSU will record time information for the first measurement, and thereafter for every first measurement after midnight. The clock features automatic leap year compensation.

Data Storage Unit 2990

The Data Storage Unit (DSU) is a portable, reusable, solid state module for storing data in the 10-bit PDC-4 code.




Engineering Data Graph from Data Reading Program 5059

When the unit is connected to a data collecting system, the display reading will increment by one every time a ten-bit data word enters the unit. The DSU 2990E can accept up to 262100 individual ten-bit words. When the unit is full, the input port is blocked, disallowing further data to be stored. A special version, designated 2990X, will continue to receive new data and delete the oldest ones. A third version, designated 2990A is a special version storing data in the PDC-0.2 code.


The data stored in the DSU is transferred to a computer by means of the DSU Reader 2995 and Data Reading Program DRP 5059 which will allow for analysis of the data or transfer to other media. The reading process will not erase the data stored and the LCD module will show the full number of stored data after the unit is disconnected. In order to erase data a specific computer command must be given.

The Data Storage Unit will, while connected to a data logging system, be supplied with power from that system. It will draw about 3 mA from the system during storage sequence, four seconds per channel, and about 0.1 mA when the system is quiescent.

Specifications 2990

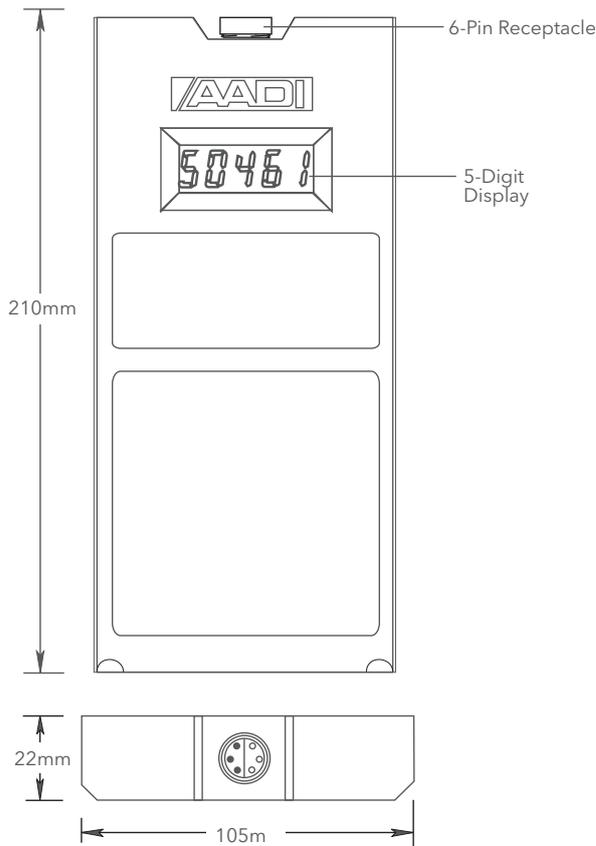

PIN CONFIGURATION

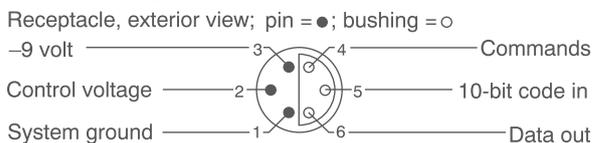

SERIAL OUTPUT FORMAT

| One Data Word, 7 characters | | | | | | | Fault | Synch |
|---|---|---|---|-------|-------|------|-----------------------|-------|
| 1 | 2 | 3 | 4 | 5 | 6 | 7 | | |
| READING (any number from 0000 to 1023) | | | | Space | Space | Null | No fault, no Synch | |
| | | | | Space | CR | LF | No fault, Synch | |
| | | | | * | Space | Null | Fault, no Synch | |
| | | | | * | CR | LF | Fault, Synch | |

Input Signal:
Output Signals:
(Commands)

10-bit binary code PDC-4
Serial, asynchronous ASCII
code at 9600 bits/s, 8 data
bits, no parity, 2 stop bits.
Mark: 0 V, Space: -5 V
Please refer to Technical
Description No. 145: "Reading
of Stored Data from DSU
2990" for a detailed account of
output format and command
specifications.

Clock stability:

±2s/day, -10 to +45°C
Time record format and
commands for clock reading
and setting are dealt with in
Technical Description No. 145.

Current Consumption:
Quiescent:
Embedded Battery:

When recording: 3mA
0.1mA
Powers clock and LCD for
>7 years

Memory Capacity:

DSU 2990A: 262,100 10-bit words
DSU 2990E : 262,100 10-bit words
DSU 2990X: 262,100 10-bit words with
overflow

Display for 2990A/E/X:


0:0000=+100000 words i.e, 6:2100 = 162100 words
0:0:000=+200000 words i.e, 6:2:100 = 262100 words
Operating Temperature: -40 to +60C (LCD becomes
illegible below -15°C)

Electrical Connection:

6-pin receptacle mating
Watertight Plug 2828

Material and Finish:

Molded

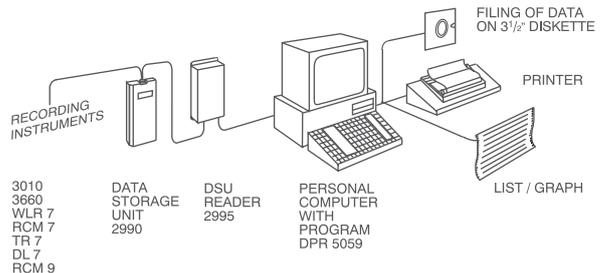

DATA READING

To read stored data the Data Storage Unit (DSU) must be interfaced to the RS-232C port of a computer by means of a DSU Reader 2995. This reader converts the 0 and -5 V serial signals from the DSU to dual-polarity signals in accordance with the RS-232 standard. In addition it supplies the power to the DSU during the read-out process. For further details refer to Data Sheet D 192. The Data Reading Program DRP 5059 is available for presenting and processing raw data. Emphasized has been put on ease of use together with versatile, graphical user interface and system flexibility. See our Web site for further details.

xylem
Let's Solve Water

Visit our Web site for the latest version
of this document and more information
www.aadi.no

Aanderaa is a trademark of Xylem Inc. or one of its subsidiaries.
© 2012 Xylem, Inc. D174 December 2012

Aanderaa Data Instruments AS
Sanddalsringen 5b, P.O. Box 103
Midtun, 5828 Bergen, Norway
Tel +47 55 60 48 00
Fax +47 55 60 48 01